# DCIEM/HPP Metabolic Measurement Software V1.0

Users' Manual



Allan Keefe Jan Pope

Defence and Civil Institute of Environmental Medicine 1133 Sheppard Ave W, P.O. Box 2000 North York, Ontario Canada, M3M 3B9

DTIC QUALITY INSPECTED 2

©HER MAJESTY THE QUEEN IN RIGHT OF CANADA (1997) as represented by the Minister of National Defence

©SA MAJESTE LA REINE EN DROIT DU CANADA (1997) Défense Nationale Canada

DEPARTMENT OF NATIONAL DEFENCE - CANADA

9970916 035

DISTRIBUTION STATEMENT A

Approved for public release; Distribution Unlimited

## **Executive Summary**

Measurement of metabolic parameters at rest and exercise is fundamental to the research conducted by the members of the Human Performance and Protection Sector of DCIEM. These data are normally measured by a metabolic measurement system consisting of gas analysers, a flow transducer and computer based data acquisition. Currently, there are numerous variations of hardware and software in use by the sector. As the operator must become familiarized with a variety of systems, the problems of inter-system variability and operator error are introduced. Furthermore, the compiled software was not malleable or available for verification of the metabolic calculations. As a result of these concerns, a new customized metabolic measurement software was developed. This software can be easily configured to work with any hardware system, is easy to learn, and adaptable to any future requirements. The following documentation is intended as a user manual, detailing the operation of the DCIEM/HPP Metabolic Measurement Software v 1.0.

## **Table of Contents**

EXECUTIVE SUMMARY	I
INTRODUCTION	1
GETTING STARTED	1
MAIN SCREEN OVERVIEW	2
VIEW INPUTS	3
CALIBRATE	4
1. Flow calibration	4
2. Gas Calibration	5
STRESS TEST	7
1. Data Screen	7
2. Menu bar 2.1. File 2.2. Subject Information 2.3. Environmental Data 2.4. Test Setup 2.5. Variables Displayed 2.6. Data Collection  3. Validation and Reliability of the System	8 8 10 10 11 12 13
<ul><li>3.1. Validation of the System</li><li>3.2. Reliability of the System</li></ul>	14 16
APPENDIX A	17
APPENDIX B	19
APPENDIX C	21
ACKNOWI EDGMENTS	24

## <u>List of Figures</u>

FIGURE 1. PROGRAM MANAGER ICON	1
FIGURE 2. MAIN MENU	2
FIGURE 3. VIEW INPUTS SCREEN	3
FIGURE 4. FLOW VOLUME SCREEN	4
FIGURE 5. FLOW CALIBRATION SCREEN	5
FIGURE 6. GAS CALIBRATION GASES	5
FIGURE 7. GAS CALIBRATION VOLTAGES	6
FIGURE 8. GAS CALIBRATION SUMMARY SCREEN	6
FIGURE 9. DATA SCREEN	7
FIGURE 10. DATA SCREEN MENU BAR	8
FIGURE 11. OPEN PREVIOUS TEST DATA (.DAT) DIALOG BOX	8
FIGURE 12. SAVE METABOLIC DATA (.MMS) DIALOG BOX	9
FIGURE 13. SUBJECT INFORMATION SCREEN	10
FIGURE 14. ENVIRONMENTAL DATA SCREEN	10
FIGURE 15. TEST SETUP SCREEN	11
FIGURE 16. VARIABLES DISPLAYED SCREEN	12
FIGURE 17 SAMPLE DATA COLLECTION SCREEN DURING A TEST.	13
FIGURE 18 SAMPLE PRINTED TEST DATA	14
FIGURE 19. VALIDATION OF THE SYSTEM	15
FIGURE 20. RELIABILITY OF THE SYSTEM	16
FIGURE 21 SCHEMATIC OF THE METABOLIC MEASUREMENT SYSTEM HARDWARE	20

## **INTRODUCTION**

The DCIEM/HPP Metabolic Measurement System (MMS) software is a MS Windows program designed to run on any IBM-PC compatible computer which has at least 4 MB of RAM and a Keithly Metrabyte DAS-8 or 800 series A/D board installed. This software was designed to provide a standardized, user-friendly and customizable system for metabolic data collection. A further advantage is its capabilities of using almost any model of gas analysers and ventilation monitors in the DCIEM inventory with little, if any, modifications to the software.

## **GETTING STARTED**

Starting the program is as simple as double clicking on the MMS icon located on the Windows Program Manager (Fig. 1).




Figure 1. Program manager icon

Upon launching the program, the first screen that you will be presented with is the "Main Menu" (Fig. 2).

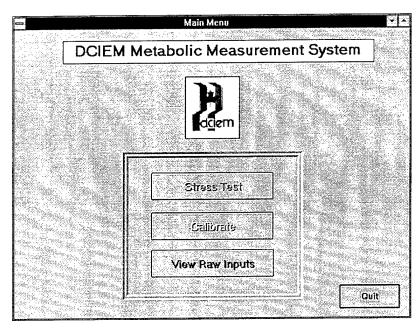


Figure 2. Main menu

From this screen, you will be able to navigate through the three primary components of this software. The options that you are presented with are as follows:

1) Stress Test Perform an exercise stress test and collect subjects' metabolic data

2) Calibrate Calibrate gas analyzers and flow transducer

3) **View Raw Inputs** Displays the current value of all analog channels and counters in real time, to verify proper functioning of each apparatus.

#### MAIN SCREEN OVERVIEW

In order to ensure accurate and trouble-free data collection, it is recommended that the user follow the sequence of verification (**View Raw Inputs**), calibration (**Calibrate**) and then data collection (**Stress Test**). Following these procedures in the sequence described will greatly enhance the probability of a successful test and simplify any troubleshooting efforts which may be required.

#### **VIEW INPUTS**

	View Input	S
Status Result Loading		
Acquired Value -5.002442	O2 Volts	<u>Channel</u>
-5.002442	CD2 Volts	1
D	Breath Switch	0 = no breath 5 = breath
Flow Counter		# Breaths 0

Figure 3. View inputs screen

Viewing inputs allows real-time simultaneous monitoring of all analyser voltages and flow transducer inputs. It is best used as a troubleshooting aid and system check to validate the proper functioning of all devices **before each metabolic run**.

Once you are satisfied that all gas analysers and the flow transducer are correctly connected to the metabolic interface box, which is in turn connected to the DAS 800 A/D card in the computer via the 32 pin cable, vary the outputs of the gas analysers by drawing an expired breath through them, or push air through the ventilation monitor. You should notice the changing voltage and pulse outputs being reflected on the "View Inputs" screen (Fig. 3). If any of the channels are not being properly updated, check all cables for proper connections. If you must disconnect any cables, please exit Windows and turn off the computer. The data acquisition card is very sensitive to electrical spikes and is easily damaged. Rebooting the computer has the added advantage of resetting any hardware or software problems which may have been responsible for invalid readings.

### **CALIBRATE**

Calibration routines are provided for both the flow transducer and gas analysers.

## 1. Flow calibration

Flow calibration requires counting the number of pulses generated by the flow transducer for a given volume of air. The volume of the calibration syringe is entered on the "Flow Volume" (Fig. 4).

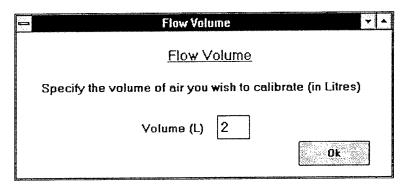


Figure 4. Flow volume screen

This volume of air is introduced through the flow transducer at a known rate. This flow rate is normally matched to the ventilation levels measured during the actual stress test (resting, walking, maximal exercise). The default flow rate for the stress test calibration is 50 L/min. Various rates can be calibrated by selecting the flow rate spin buttons (up/down arrows) (Fig 5.). This will affect the rate of the animation sequence of the syringe icon. By using a calibrated syringe to introduce the flow into the transducer, and following the animated icon, the required flow rate can be accurately produced.

Clicking on "Begin Flow" resets the # of pulses counted to 0, initiates the animated icon and begins measuring the pulse output from the flow transducer. Once the desired volume of air has been pushed through the flow transducer, clicking "Flow Complete" will display the number of pulses that have been counted. Depending on the configuration of the KL Engineering flow transducers, one should expect in the order of either 100 (normal) or 123 (high resolution) pulses per litre of air.

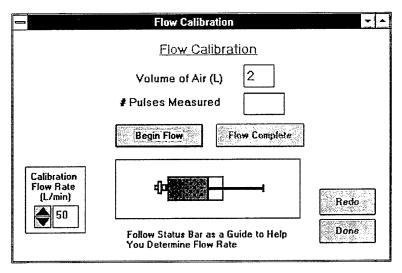


Figure 5. Flow calibration screen

## 2. Gas Calibration

Gas Calibration requires the flow of two previously calibrated gases through the gas analysers. As each gas is introduced, the user is prompted to enter the current  $O_2$  and  $CO_2$  concentrations (Fig. 6). Upon clicking "Calibrate", the gas analysers are read by the data acquisition system (Fig. 7), and a calibration slope and intercept are calculated. The calibration slope and intercept are utilized by the MMS software to convert the voltage outputs from the  $O_2$  and  $CO_2$  analysers to known gas concentrations.

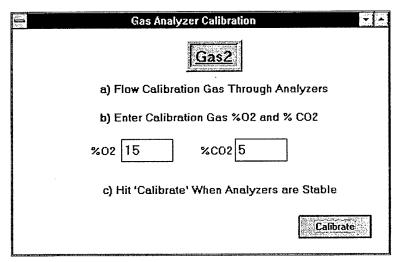


Figure 6. Gas calibration gases

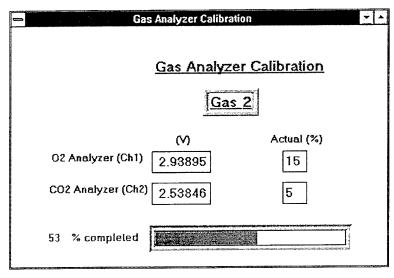


Figure 7. Gas calibration voltages

After the second gas is analysed, a summary report is generated which displays the data from the calibration (Fig. 8). This information is useful for verification of the quality of the calibration. For instance, the Ametek S-3A analyzer output range is 0 to 5V for 0 to 25%  $O_2$ , while the Ametek CD-3A's output range is 0 to 5V for 0 to 10%  $CO_2$ . Thus a calibration gas of 15%  $O_2$  and 5%  $CO_2$  should result in an output of 3V and 2.5V respectively. If the calibration summary is suspect, the entire calibration procedure maybe repeated by clicking 'Recalibrate'.

4000 4000 4000 4000		Gas Calil	ration Summary				
Summary of Gas Analyzer Calibration							
		Actual %	Volts	% / Volts			
	02	21	4.1102	5.1092			
Gas 1	CO2	0	0.0164	<b>O</b> .			
00	02	15	2.9381	5.1053			
Gas 2	C02	5	2.5327	1.9741			
		je joj	Re	calibrate			
		S. Bernson		3.			

Figure 8. Gas calibration summary screen

### STRESS TEST

The stress test portion of the program is designed to be as simple, user-friendly, and customizable as possible. Although there are necessary anthropometric and environmental data which must be determined before each test, these may be saved to a file for recall, and modified as required for subsequent tests.

## 1. Data Screen

Upon clicking "Stress Test" from the "Main Menu" screen, you are presented with the following form:

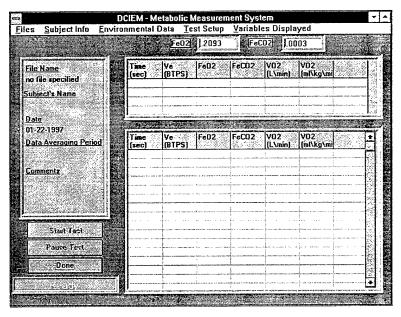


Figure 9. Data screen

The left information box displays a summary of the current test, while the grids to the right display the metabolic data as they are collected. The top grid gives a continuous 15 second averaged update of metabolic data, while the bottom grid is updated with averages according to 15, 30 or 60 second default options or a user defined period (in minutes). It is the data appearing in the bottom grid which may be stored on disk or printed. This must be specified prior to data collection (see Test Setup). The bottom left status window (Ready) indicates whether all required test data have been entered before the test is

allowed to proceed. FeO<sub>2</sub> and FeCO<sub>2</sub> are also continuously updated for monitoring purposes during the test.

## 2. Menu bar



Figure 10. Data screen menu bar

The menu bar (Fig. 10) contains the subject, environmental and test options that you will need to complete before initiating collection of metabolic data. These data are best entered by selecting each option from left to right and completing the requested data screens.

#### 2.1. File

This menu item allows the retrieval and storage of subject, environmental and test setup data. Test data are stored in two files having the syntax <filename.DAT> and <filename.MMS>. These files are only created when the user wishes to save the metabolic data to a file (see Test Setup). The files with the ".DAT" extensions contain all the relevant test parameters, while the files with the ".MMS" extensions are tab delimited text files containing the actual metabolic data. This data can be retrieved by any spreadsheet or text editor. By clicking on "File...Open", the following dialog box appears, prompting the user to select previous test parameters.

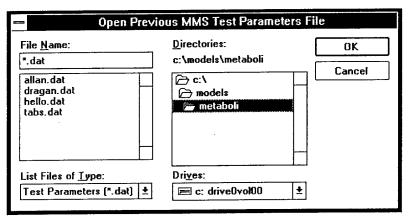


Figure 11. Open previous test data (.DAT) dialog box

If the software detects that the previous test parameters requested the data to be saved to a file, a second dialog box will appear, prompting the user to enter a filename for the data to be stored.

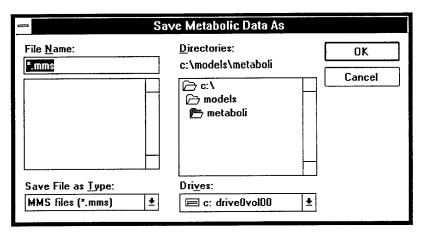


Figure 12. Save metabolic data (.MMS) dialog box

**Note:** It is not necessary to type in the .MMS or .DAT extensions. They will be appended to the filename automatically.

The file menu options also include "File...Save .DAT File" which allows the user to save only the test parameters, without the creation of a .MMS file, and a "File...Exit" option which returns the program to the **Main Screen**.

## 2.2. Subject Information

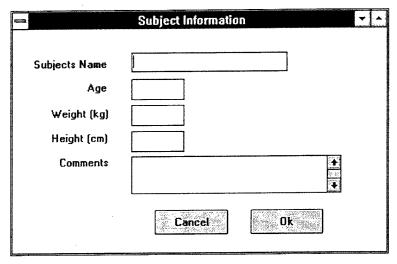


Figure 13. Subject information screen

This screen allows the user to input anthropometric and general identification information regarding the subject. **Note: Age, weight** and **height** are required information, and the stress test program will not run without this information.

#### 2.3. Environmental Data

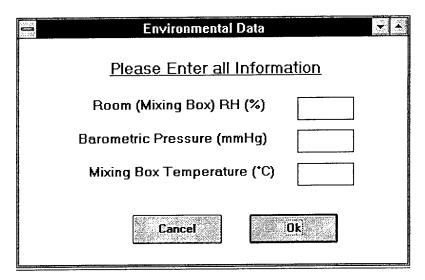


Figure 14. Environmental data screen

Environmental parameters are entered on this form. All of this data is required to proceed with the test. Please note that since expired ventilation is being measured, the relative humidity and temperature inputs should be from the **mixing box**, not the ambient environment. Mixing box relative humidity is assumed to be 100% for expired air. For tests conducted at normal room temperatures of 20 to 25 °C, a mixing box temperature of 25 °C is used. Alternatively, the mixing box temperature may be measured directly with a thermistor during pilot studies.

## 2.4. Test Setup

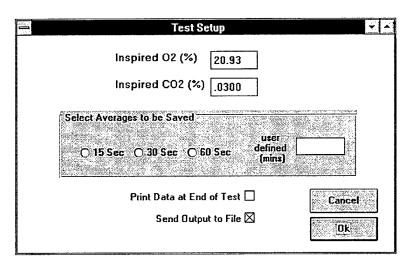


Figure 15. Test setup screen

Various parameters selected on the "Test Setup" screen allow the user greater customization of how the test is performed.

If gas mixtures other than room air are being used, then the new inspired percent  $O_2$  and  $CO_2$  may be entered at this point. Otherwise, the default values of 20.93%  $O_2$  and .03%  $CO_2$  will be used for the test.

Data averaging is determined by choosing either one of the three default options (15, 30 or 60 second periods), or as defined by the user (in minutes). This option controls the updating of the second larger grid on the stress test display.

Finally, the last two options allow the user control of the test results output. None, one, or both of these output options may be selected. By selecting "Send Output to File" all of the stress test data calculated, whether displayed or

not, will be sent to an MS Excel-compatible tab-delimited file. You will be prompted for a file name and path if this option is selected.

If a printed report is required, simply click this option and a full report will be generated at the end of the test. This report contains **only the data selected to be displayed**. See section 2.5 Variables Displayed for more detail. **Important:** make sure that a printer is properly connected, turned on and selected by the Print Manager as the default printer, or you may experience problems printing your data. If in doubt, it is always safest to save the file to disk.

## 2.5. Variables Displayed

Variables Displayed				
Select the Variables You Wish to Display (max 6)				
☐ Ve (btps)	☐ VCO2 (ml/kg/min)			
⊠ Ve (stpd)	⊠ RER			
⊠ Fe02	☐ Met Rate (Watts)			
⊠ FeCO2	☐ V02/Ve			
⊠ VO2 (L/min)	☐ VC02/Ve			
☑ VCO2 (L/min)	Freq (breath/min)			
☐ VO2 (ml/kg/min)				
(Ok	Cancel			

Figure 16. Variables displayed screen

The "Variables Displayed" screen allows the user to customize the display grids to monitor the metabolic variables most relevant to the particular test. A maximum of six variables may be selected; however, one can return to this screen at any time during the ongoing test and reselect the variables. The grids will reflect this change only from the latest reading.

#### 2.6. Data Collection

Figure 17 illustrates the "Data Screen" during a typical test. In this example, the current test summary data appears in the left information box, while the 15 second updates appear in the upper grid. In this test, metabolic data were calculated as minute averages every 30 seconds. These data appear in the lower grid. Note that the data appearing on the grids were determined by the "Variables Displayed" screen illustrated by figure 16.

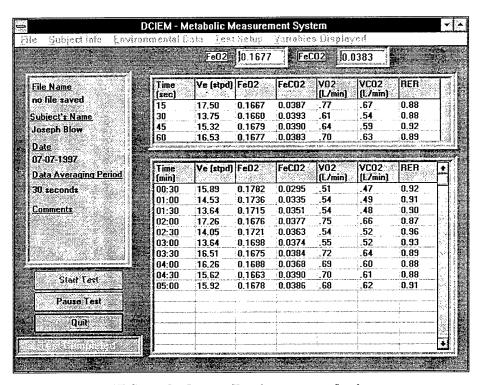


Figure 17 Sample data collection screen during a test.

If the printed output option is selected, a printout of the test data will be produced at the conclusion of data collection (Figure 18). Again, the data printed are those selected from the "Variables Displayed" screen (Figure 16). For a more comprehensive record of metabolic data variables, save the data to file.

#### DCIEM Metabolic Measurement System

Test Date: 07-07-1997

File Name:

Subject's Name: Joseph Blow

Height (cm): 180

Weight (kg): 77

Age: 35

Barometric Pressure (mmHg): 760

Mixing Box Temperature (C): 25

Mixing Box RH (%): 100

#### Comments:

Time (min)	Ve (stpd)	FeO2	FeCO2	VO2 (L/min)	VCO2 (L/min)	RER
00:30	15.89	0.1782	0.0295	.51	.47	0.92
01:00	14.53	0.1736	0.0335	.54	.49	0.91
01:30	13.64	0.1715	0.0351	.54	.48	0.90
02:00	17.26	0.1676	0.0377	.75	.66	0.87
02:30	14.05	0.1721	0.0363	.54	.52	0.96
03:00	13.64	0.1698	0.0374	.55	.52	0.93
03:30	16.51	0.1675	0.0384	.72	.64	0.89
04:00	16.26	0.1688	0.0368	.69	.60	0.88
04:30	15.62	0.1663	0.0390	.70	.61	0.88
05:00	15.92	0.1678	0.0386	.68	.62	0.91

Figure 18 Sample printed test data

## 3. Validation and Reliability of the System

## 3.1. Validation of the System

Four males and three females performed five minutes of exercise on a bicycle ergometer at each of five increasing workloads. The metabolic system described was connected in series with a Tissot gasometer and Ametek oxygen and carbon dioxide analysers, the latter being considered the "gold standard" for such measurements. The last minute of exercise at each workload was used to collect expired air in the gasometer for subsequent analyses of ventilation and expired gas concentrations. Oxygen consumption was calculated in accordance with well established equations for open circuit spirometry. Figure 19 depicts a scattergram of oxygen consumption for the "cart" vs. the "tissot". A Fisher's F-test indicated no significant difference between the two systems and the line of identity. Therefore, this new software/hardware system can be considered to be valid and accurate.

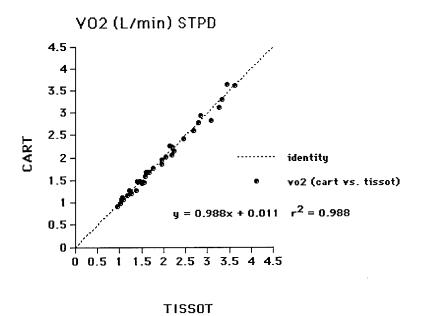


Figure 19. Validation of the System

## 3.2. Reliability of the System

Five males performed a maximal oxygen consumption test on a treadmill as a pre-requisite for participation in a heat stress experiment. The protocol consisted of running at a self-determined speed with an increase in grade of 1% per minute until exhaustion. After completion of the heat stress trial, a "post" determination of maximal oxygen consumption was performed in exact accordance to the "pre" evaluation. Figure 20 depicts a scattergram of oxygen consumption for the "pre" vs. the "post" trials at the same treadmill speeds and % grade during the incremental test. A Fisher's F-test indicated no significant difference between the two days and the line of identity. This new software/hardware system can be considered to be reliable and reproducible.

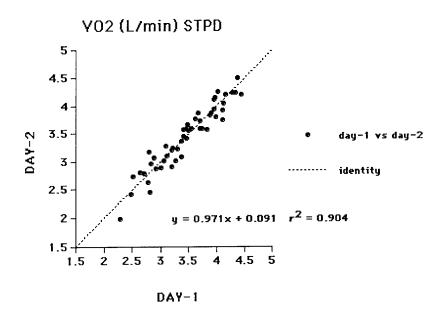


Figure 20. Reliability of the System

Appendix A

Pin Out Tables

## DAS 8/800 main I/O connector (37 pin)

<u>Pin number</u>	<b>Function</b>	Variable Measured
2	clk 0	flow
12 to 18	low level	ground
29	common +5V	+5V to flow transducer
37	analog ch 1	$^{\circ}$ O <sub>2</sub>
36	analog ch 2	$^{\circ}CO_{2}$
35	analog ch 3	respiration

## KL Engineering KTC-3D

Pin Number	<u>Variable</u>		
2	Power supply ground		
4	flow (100 PPL)		
5	flow (123 PPL)		
6	Respiration (0-5 V)		
7	Power supply +5V		

Appendix B

**Hardware Schematics** 

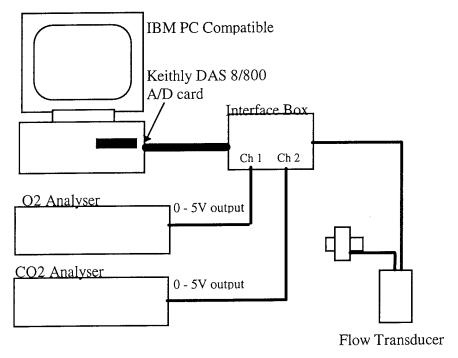


Figure 21.Schematic of the Metabolic Measurement System Hardware

Appendix C

**Metabolic Calculations** 

## Summary of metabolic formulae used in the calculation of metabolic data.

$$F_1N_2 = 1 - (F_1CO_2 + F_1O_2)$$

$$F_EN_2 = 1 - (F_ECO_2 + F_EO_2)$$

$$\dot{V}_{I(ATP)} = \dot{V}_{E(ATP)} \times \frac{F_E N_2}{F_I N_2} \tag{lemin}^{-1}$$

$$\dot{V}_{E(BTPS)} = \dot{V}_{E(ATP)} \times \frac{(273.23 + T_B)}{(273.23 + T_A)} \times \frac{(P_B - P_{H2O(A)})}{(P_B - P_{H2O(B)})}$$
 (1•min<sup>-1</sup>)

$$\dot{V}_{E(STPD)} = \dot{V}_{I(STPD)} \times \frac{F_I N_2}{F_E N_2}$$
 (1•min<sup>-1</sup>)

$$\dot{V}O_2 = \dot{V}_{I(STPD)} \times (F_IO_2) - (\dot{V}_{E(STPD)} \times F_EO_2)$$
 (1•min<sup>-1</sup>)

$$\dot{V}CO_2 = \dot{V}_{E(STPD)} \times (F_ECO_2) - (\dot{V}_{I(STPD)} \times F_ICO_2)$$
 (1•min<sup>-1</sup>)

$$RQ = \frac{\dot{V}CO_2}{\dot{V}O_2}$$

$$Energy = 352 \times (.23 \times RQ + .77) \times \dot{V}O_2 \tag{W}$$

$$SA = .202 \times wt^{-425} \times ht^{-725}$$
 (m<sup>2</sup>)

$$P_{H^2O(A)} = 4.579 \times 10^{\frac{7.5 \times T_A}{T_A + 273.23}} \times \frac{RH}{100}$$
 (mmHg)

$$P_{H_{2O(B)}} = 4.579 \times 10^{\frac{7.5 \times T_B}{T_B + 273.23}}$$
 (mmHg)

#### Where:

 $F_1N_2$  = Inspired fraction

 $F_E N_2 = Expired fraction$ 

 $\dot{\mathbf{V}}_{\mathbf{I}}$  = Inspired minute ventilation

 $\dot{\mathbf{V}}_{\text{E}} = \text{Expired minute ventilation}$ 

STPD = Standard temperature and pressure, dry

**ATPS** = Ambient temperature and pressure, saturated

 $P_B = Barometric pressure (mmHg)$ 

**RH** = Relative humidity (%)

SA = Body surface area (m<sup>2</sup>)

wt = body weight (kg)

ht = height (m)

 $P_{H2O(x)}$  = Water vapour pressure (ambient or body temperature)

 $T_A$  = Ambient temperature (°C)

 $T_B = Body temperature (37°C)$ 

## Acknowledgments

The authors would like to thank Dr. P Tikuisis for his assistance with the statistical analysis of the validity and reliability data, and Dr. T McLellan for his physiological and editing expertise.

# SECURITY CLASSIFICATION OF FORM (Highest classification of Title, Abstract, Keywords)

DOCUMENT CONTROL DATA (Security classification of title, body of abstract and indexing annotation must be entered when the overall document is classified)					
1. ORIGINATOR (the name and address of the organization preparing the document. Organizations for whom the document was prepared, e.g., Establishment sponsoring a contractor's report, or tasking agency, are entered in section 12.)		DOCUMENT SECURITY CLASSIFICATION (overall security classification of the document including special warning terms if applicable)			
DCIEM 1133 Sheppard Ave W. Downsview, Ont. M3M 3B9				Unclassified	
3. DOCUMENT TITLE (the complete documer abbreviation (S,C,R or U) in parentheses after the DCIEM/HPP Metabolic Measurement Software).	e title.)		fication sh	ould be indicated be the appropriate	
4. DESCRIPTIVE NOTES (the category of the report, e.g. interim, progress, summary, annual o	document, e.g., technicar final. Give the inclusiv	l report, technical no e dates when a specif	te or mem	orandum. If appropriate, enter the type of ng period is covered.)	
Technical memorandum	: ':: 1 T6 -: '!' h	mark o a Duma Ma	: Conle E	)	
5. AUTHOR(S) (Last name, first name, middle Keefe, Allan A. Pope, J	initial. If military, snow	rank, e.g. Burns, Ma	ј. гтапк в	.)	
6. DOCUMENT DATE (month and year of publication of document)  July 97	7.a. NO. OF PAGES (total containing information. Include Annexes, Appendices, etc.) 23		mation.	7.b. NO. OF REFS. (total cited in document)	
8.a. PROJECT OR GRANT NO. (if appropriate, the applicable research and development project or grant number under which the document was written. Please specify whether project or grant)  8.b. CONTRACT NO. (if appropriate, the applicable number under which the document was written)					
9.a. ORIGINATOR'S DOCUMENT NUMBER (the official document number by which the document is identified by the originating activity. This number must be unique to this document.)  9.b. OTHER DOCUMENT NO.(S) (any other numbers which may assigned this document either by the originator or by the sponsor.)					
10. DOCUMENT AVAILABILITY (any limitation on further dissemination of the document, other than those imposed by security classification)  x Unlimited distribution Distribution limited to defence departments and defence contractors; further distribution only as approved Distribution limited to defence departments and Canadian defence contractors; further distribution only as approved Distribution limited to government departments and agencies; further distribution only as approved Distribution limited to defence departments; further distribution only as approved Other					
11. ANNOUNCEMENT AVAILABILITY (any limitation to the bibliographic announcement of this document. This will normally correspond to the Document Availability (10.) However, where further distribution (beyond the audience specified in 10) is possible, a wider announcement audience may be selected.)					
12. SPONSORING ACTIVITY (the name of the department project office or laboratory sponsoring the research and development. Include the address.)					

DSIS DCD03 HFD 09/94

Undaci.

SECURITY CLASSIFICATION OF FORM (Highest classification of Title, Abstract, Keywords)

## Undais.

## SECURITY CLASSIFICATION OF FORM (Highest classification of Title, Abstract, Keywords)

13. ABSTRACT (a brief and factual summary of the document. It may also appear elsewhere in the body of the document itself. It is highly desirable that the abstract of classified documents be unclassified. Each paragraph of the abstract shall begin with an indication of the security classification of the information in the paragraph (unless the document itself is unclassified) represented as (S), (C), (R), or (U). It is not necessary to include here abstracts in both official languages unless the text is bilingual).

Measurement of metabolic parameters at rest and exercise is fundamental to the research conducted by the members of the Human Performance and Protection Sector of DCIEM. These data are normally measured by a metabolic measurement system consisting of gas analysers, a flow transducer and computer based data acquisition. Currently, there are numerous variations of hardware and software in use by the sector. This introduces the problems of intersystem variability, and operator error, as the unique procedures for operating each system must become familiarized. Furthermore, the compiled software was not malleable or available for verification of the metabolic calculations. As a result of these concerns, a new customized metabolic measurement software was developed. This software can be easily configured to work with any hardware system, is easy to learn, and adaptable to any future requirements. The following documentation is intended as a user manual, detailing the operation of the DCIEM/HPP Metabolic Measurement Software v 1.0.

14. KEYWORDS, DESCRIPTORS or IDENTIFIERS (technically meaningful terms or short phrases that characterize a document and could be helpful in cataloguing the document. They should be selected so that no security classification is required. Identifiers, such as equipment model designation, trade name, military project code name, geographic location may also be included. If possible, keywords should be selected from a published thesaurus, e.g. Thesaurus of Engineering and Scientific Terms (TEST) and that thesaurus identified. If it is not possible to select indexing terms which are Unclassified, the classification of each should be indicated as with the title.)

Metabolism, exercise,  $\dot{V}O_2$ , oxygen uptake, respiratory gas analysis.

DSIS DCD03 HED 07/94

undacs

SECURITY CLASSIFICATION OF FORM (Highest classification of Title, Abstract, Keywords)